


How to set up the Olympus Confocal for polarization microscopy

1. Pull DIC slider (under stage) out
2. Push slider polarizer in (above the condenser). Can loose the knob first and adjust in or out to get different darkness levels

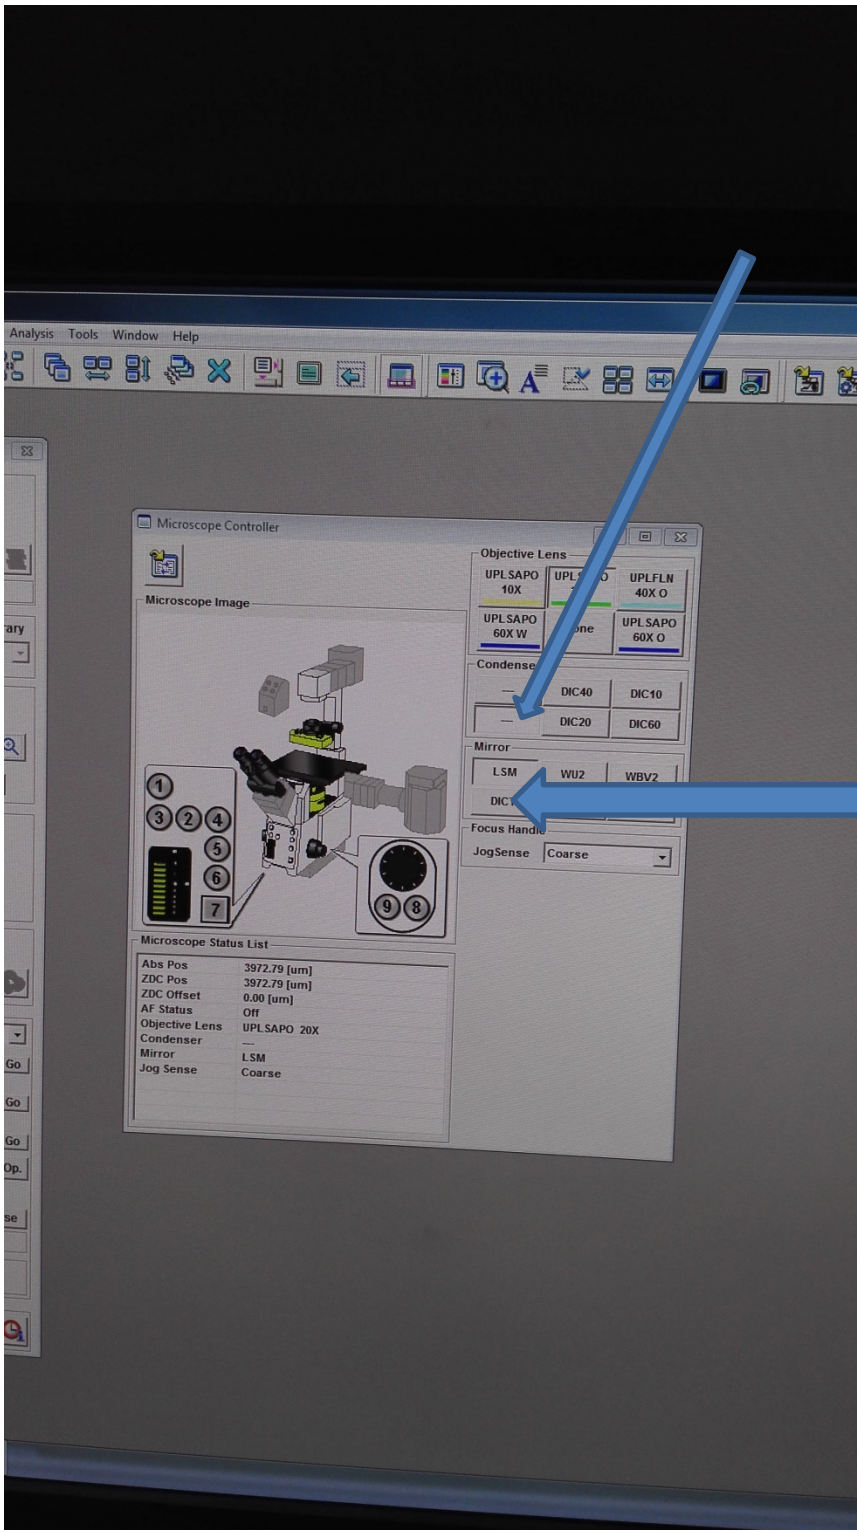

Condenser position:
click “—” (not DIC
one)

Click “DICT” (not “LSM”).

When imaging, use 473
laser and DIC channel to
take image as usual.